

201-395.02  
202-164.00(4)

A

THE COMMISSIONER OF PATENTS AND TRADEMARKS  
WASHINGTON, D.C. 20231

Case Docket No.: 172/19

02/26/98  
535 U.S. PTO

Submitted herewith for filing is the patent application of

For: GIDEON SHENHOLZ AND YITZHAK ZLOTER

For: PRESENTATION BOARD DIGITIZER SYSTEMS

Enclosed are:

- ☒ 12 sheets of informal drawing(s).
- ☒ An assignment of the invention to PEGASUS TECHNOLOGIES LTD.
- ☐ A certified copy of a \_\_\_\_\_ application.
- ☐ An associate power of attorney.
- ☒ A verified statement to establish small entity status under 37 CFR 1.9 and 37 CFR 1.27.
- ☐ Other - \_\_\_\_\_

The filing fee has been calculated as shown below:

	(Col.1) NO. FILED	(Col.2) NO. EXTRA
FOR:		
BASIC FEE		
TOTAL CLAIMS	19 - 20=	
INDEP CLAIMS	7 - 3=	4
... Recordal of Assignment		40

SMALL ENTITY	
RATE	FEE
	\$ 395
x11=	\$
4 x41	\$ 164
	\$ 40
TOTAL	\$ 599

OTHER THAN A SMALL ENTITY	
RATE	FEE
	\$ 790
x22=	\$
x82	\$
	\$
TOTAL	\$

If the difference in Col.1 is less than zero, enter "0" in Col.2

- ☒ Please charge my Deposit Account No. 06-2140 in the amount of \$ 599. A duplicate copy of this sheet is enclosed.
- ☐ A check in the amount of \$ \_\_\_\_\_ to cover the filing fee is enclosed.
- ☒ The Commissioner is hereby authorized to charge payment of the following fees associated with this communication or credit any overpayment to Deposit Account No. 06-2140. A duplicate copy of this sheet is enclosed.
  - ☒ Any additional filing fees required under 37 CFR 1.16.
  - ☒ Any patent application processing fees under 37 CFR 1.17.
- ☒ The Commissioner is hereby authorized to charge payment of the following fees during the pendency of this application or credit any overpayment to Deposit Account No. 06-2140. A duplicate copy of this sheet is enclosed.
  - ☒ Any patent application processing fees under 37 CFR 1.17.
  - ☐ The issue fee set in 37 CFR 1.18 at or before mailing of the Notice of allowance, pursuant to 37 CFR 1.311(b).
  - ☒ Any filing fees under 37 CFR 1.16 for presentation of extra claims.

Respectfully,

Mark M. Friedman  
Reg. No. 33,883

Mark M. Friedman  
DR. MARK FRIEDMAN LTD.  
C/O Anthony Castorina  
2001 Jefferson Davis Highway  
Suite 207  
Arlington, Virginia 22202

IN THE UNITED STATES PATENT AND TRADEMARK OFFICEIn RE Application of: GIDEON SHENHOLZ AND YITZHAK ZLOTER

Filed Concurrently Herewith

For: PRESENTATION BOARD DIGITIZER SYSTEMSVERIFIED STATEMENT UNDER 37 CFR 1.27  
CLAIMING STATUS AS A SMALL ENTITY

To The Commissioner of Patents and Trademarks:

I hereby declare that:

I am the owner of, or an official empowered to act on behalf of, the small business concern identified below:

Name of Concern: PEGASUS TECHNOLOGIES LTD.Address : P.O. BOX 23144, 61231 TEL AVIV, ISRAEL

The small business concern identified above, together with its affiliates, employs fewer than 500 persons and qualifies as a small business concern as defined in 37 CFR 1.9(d) for purposes of paying reduced fees under 35 USC § 41(a) and § 41(b) to the Patent and Trademark Office with regard to the above-entitled invention described in the specification filed herewith.

Rights under contract or law have been conveyed to and remain with the small business concern identified above with regard to the above entitled invention.

If the rights held by the small business concern are not exclusive, each other party having rights to the invention is listed below, and no rights to the invention are held by any party who could not qualify as a small entity under 37 CFR 1.9(f), namely any person who could not be classified as an independent inventor under 37 CFR 1.9(c) if that person had made the invention, or any concern which would not qualify as a small business concern under 37 CFR 1.9(d) or a nonprofit organization under 37 CFR 1.9(e).

Full Name (Party 1): NONE

Address : \_\_\_\_\_

Status : ☐ Individual ☐ Small Business Concern ☐ Nonprofit Organization

Full Name (Party 2): \_\_\_\_\_

Address : \_\_\_\_\_

Status : ☐ Individual ☐ Small Business Concern ☐ Nonprofit Organization

I acknowledge the duty under 37 CFR 1.28(b) to file, in this application, notification of any change in status resulting in loss of entitlement to small entity status prior to paying, or at the time of paying, the issue fee due after the date on which status as a small entity is no longer appropriate.

I hereby declare that all statements made herein of my own knowledge are true and that all statements made on information and belief are believed to be true; and further that these statements were made with the knowledge that willful false statements and the like so made are punishable by fine or imprisonment, or both, under Section 1001 of Title 18 of the United States Code, and that such willful false statements may jeopardize the validity of the application and any patent issuing thereon.

GIDEON SHENHOLZ  
Name of Person Signing

Signature [Signature]

23.2.98  
Date

Capacity of Person Signing: DIRECTORAddress of Person Signing : 2 HAEKODEI, 64073 TEL AVIV, ISRAEL

## APPLICATION FOR PATENT

Inventors: Gideon Shenholz and Yitzhak Zloter

Title: Presentation Board Digitizer Systems

### FIELD AND BACKGROUND OF THE INVENTION

5           The present invention relates to digitizers and, in particular, it concerns devices for use with conventional presentation boards and pens for digitizing lines drawn manually.

          It is known to use various techniques for determining the position of a writing implement or stylus on a flat surface. U.S. Patents Nos. 4,564,928 to  
10   Glenn et al., 4,886,943 to Suzuki et al., 4,910,363 and 5,073,685 to Kobayashi et al. and 5,097,102 to Yoshimura et al. all disclose systems in which a vibrating element associated with a pen transmits vibrations through the material of a board. The vibrations are detected by transducers attached to the board and the position of the pen is calculated from the transmission time of the  
15   vibrations through the board. These systems inherently function exclusively when the pen is in contact with the board such that vibrations are transferred to the board. As a result, no special mechanism is required to distinguish writing from non-writing pen movements.

          These systems are generally inaccurate due to non-uniform transmission  
20   times through the board. In fact, they typically require highly specialized board structures which renders them expensive and inconvenient.

An alternative approach is the use of air-borne ultrasound signals. Examples of such systems are described in U.S. Patents Nos. 4,777,329 to Mallicoat, 4,814,552 to Stefik et al., 4,506,354 to Hansen and 4,758,691 to De Bruyne. These systems employ various combinations of ultrasound transmitters and receivers arranged at two points fixed relative to a board and on a movable writing implement. The position of the movable implement is then derived by triangulation. The systems typically require an additional hard-wired or electromagnetic link between the movable implement and a base unit to provide timing information for time-of-flight ultrasound calculations. An additional switch is also required to identify when the movable element is in contact with the board.

These systems are typically limited to relatively small boards. This is because of signal to noise ratio (SNR) limitations. The volume of ultrasound used cannot be very high without causing bothersome accompanying whistling noises. Additionally, in a wireless system, power considerations severely limit the transmitted volume. In order to generate reliable position information, the transmitter-to-receiver distance must therefore be kept small. Attempts to use different sets of receivers for different regions of a large board generally result in discontinuities when the movable element travels from one region to another.

Another shortcoming of these systems is their inability to reproduce rapid interrupted pen strokes such as performed when drawing a dashed line. Typically, the transmitter or receiver element in the pen turns off when the pen is inactive and is re-activated each time the pen comes in contact with the

board. The system then takes a fraction of a second to resynchronize before it responds correctly. In the case of short strokes, the length of the operative stroke may be comparable with the response time of the system, thereby giving very poor results.

5           An additional problem of the airborne ultrasound digitizer systems is that the ultrasound transmitter or receiver element is mounted asymmetrically to the side of the drawing implement. As a result, the measured position is offset from the true drawing position in a direction which changes with rotation of the drawing implement. This may result in discontinuities and illegible  
10       writing in the digitized image when the drawing implement position is changed between strokes.

          Finally, conventional presentation board digitizer systems are typically limited to use with specially produced writing implements. This renders them expensive since pens have a very limited lifetime. Even where the ink cartridge  
15       is separately replaceable, the components used must be of a very specific design to be compatible.

          There is therefore a need for a reliable, low-cost, digitizer system which may be used with conventional presentation boards of all sizes for determining accurately the position of a drawing implement on the board. It would also be  
20       advantageous to have a transmitter device for use with presentation board which can be used with a wide range of conventional writing implements.

## SUMMARY OF THE INVENTION

The present invention is of presentation board digitizer systems for use with presentation boards of all sizes which allow accurate reproduction of short pen strokes and which may be used with conventional writing implements.

5       According to the teachings of the present invention there is provided, an ultrasound receiver assembly for use in a presentation board digitizer system, the receiver assembly comprising: (a) a first ultrasound receiver located adjacent to the surface of the presentation board; and (b) a second ultrasound receiver displaced from the first ultrasound receiver in a direction substantially  
10       perpendicular to the surface of the presentation board, the first and second ultrasound receivers being connected so as to generate a total output signal corresponding to the instantaneous sum of the ultrasound signals received at each of the first and second ultrasound receivers such that the receiver assembly is most sensitive to ultrasound signals incident from a plane substantially  
15       adjacent to the presentation board.

      According to a further feature of the present invention, the first and second receivers are connected in series.

      In the context of an ultrasound-based digitizing system for identifying the position of an ultrasound transmitter associated with an element movable  
20       relative to a surface, the system having at least three spaced apart ultrasound receivers associated with the surface, there is also provided according to the teachings of the present invention, a method of analyzing outputs from the ultrasound receivers comprising the step of identifying as a current position a

weighted centroid of at least a first calculated position derived from the outputs of a first pair of the receivers and a second calculated position derived from the outputs of a second pair of the receivers, wherein the weighting varies as a continuous function of approximate position relative to the ultrasound receivers.

According to a further feature of the present invention, the ultrasound receivers are substantially collinear, and the weighting varies linearly with distance in the direction of alignment of the ultrasound receivers over at least a given switch-over zone.

According to a further feature of the present invention, the weighted centroid approximates to the first calculated value when the movable element is within a first given region of the surface.

There is also provided according to the teachings of the present invention, a presentation board digitizer system for digitizing operative strokes of a drawing implement carrying an ultrasound transmitter against the board, the system comprising: (a) at least two ultrasound receivers mounted relative to the board for receiving air-borne ultrasound signals; (b) a transducer associated with the board so as to detect vibrations from the transmitter conducted through the board; and (c) a processor responsive to outputs from the at least two ultrasound receivers to calculate a current position of the transmitter, the processor being additionally responsive to an output from the transducer to identify contact between the drawing implement and the board, thereby identifying operative strokes of the drawing implement.

There is also provided according to the teachings of the present invention, a transmitter device for use with a system for digitizing operative strokes of a hand-held drawing implement, the drawing implement having a body and an operative tip, the transmitter device comprising: (a) a housing having a substantially cylindrical opening terminating at a first end in an annular wedge surface with a central bore, the housing receiving a portion of the body of the drawing implement with its operative tip extending from the central bore; (b) a retainer attachable to a second end of the opening to retain the drawing implement within the housing, the retainer having a spring element for biasing the drawing implement towards the annular wedge surface; and (c) a transmitter mounted relative to the housing proximal to the central bore.

According to a further feature of the present invention, the housing further includes: (a) a microswitch actuated by changes in pressure exerted on the annular wedge surface so as to be responsive to a force exerted on the operative tip of the drawing implement towards the housing; and (b) electronic circuitry responsive to the microswitch to affect operation of the transmitter at least when the microswitch indicates a force exerted on the operative tip of the drawing implement towards the housing.

According to a further feature of the present invention, the electronic circuitry operates the transmitter for a given time interval after the microswitch ceases to indicate a force exerted on the outer housing towards the operative tip of the drawing implement.

According to a further feature of the present invention, the given time interval is at least about half a second.

According to a further feature of the present invention, the transmitter transmits continuously, and the electronic circuitry is responsive to the  
5 microswitch to change a signal transmitted by the transmitter while the microswitch indicates a force exerted on the operative tip of the drawing implement towards the housing.

According to a further feature of the present invention, the transmitter is an ultrasound transducer.

10 According to a further feature of the present invention, there are also provided elements of an electromagnetic communications link, the elements being associated with the electronic circuitry.

There is also provided according to the teachings of the present invention, an ultrasound transmitter device for use with a system for digitizing  
15 the position of a hand-held drawing implement, the drawing implement having a central axis and an operative tip, the transmitter device comprising a substantially cylindrical piezoelectric transmitter element positioned coaxially with the drawing implement so as to circumscribe a part of the drawing implement proximal to the operative tip.

20 There is also provided according to the teachings of the present invention, an eraser device for use with a presentation board digitizer system, the eraser device comprising: (a) a handle; (b) an eraser element having a substantially flat eraser surface; and (c) a pivot joint connecting between the

handle and the eraser element, the pivot joint having two degrees of rotational freedom such that, in use, the eraser element assumes an orientation with the eraser surface parallel to the presentation board surface substantially independent of the orientation at which the handle is held.

## 5 BRIEF DESCRIPTION OF THE DRAWINGS

The invention is herein described, by way of example only, with reference to the accompanying drawings, wherein:

FIG. 1 is a schematic front view of a presentation board provided with a digitizer system, constructed and operative according to the teachings of the present invention, showing a switch-over zone between regions with different groups of ultrasound receivers;

FIG. 2 is a plot illustrating the variation of relative weighting of position indications from two sets of ultrasound receivers in Figure 1 as a function of position across the presentation board;

FIG. 3 is a side view of a twin ultrasound receiver assembly for use in a presentation board digitizer system constructed and operative according to the teachings of the present invention;

FIG. 4 is a schematic representation of the reception characteristic of the twin ultrasound receiver assembly of Figure 3;

FIG. 5 is a side cross-sectional view of a transmitter device, constructed and operative according to the teachings of the present invention, used with a conventional drawing implement in a digitizer system;

FIG. 6A is an exploded perspective view of a microswitch structure, constructed and operative according to the teachings of the present invention, for use in the transmitter device of Figure 5;

FIG. 6B is a perspective view of the microswitch structure of Figure 6A assembled;

FIG. 6C is a top view of the microswitch structure of Figure 6A showing a retaining spring arrangement;

FIG. 7 is a schematic perspective view of a preferred structure for attachment of a retaining member to a housing for use in the transmitter device of Figure 5;

FIG. 8A is a plot of the output of a contact switch activated by operational contact between a drawing implement and a presentation board as a function of time;

FIG. 8B illustrates the recorded drawing implement operation time profile produced by prior art systems corresponding to the contact profile of Figure 5A;

FIG. 8C illustrates the corresponding recorded drawing implement operation time profile produced according to a first embodiment of a presentation board digitizer system, constructed and operative according to the teachings of the present invention;

FIG. 9 is a side cross-sectional view of an eraser transmitter unit, constructed and operative according to the teachings of the present invention, for use with a digitizer system;

FIG. 10 illustrates the signals received by air-borne ultrasound receivers and a board-mounted transducer, respectively, according to a second embodiment of a presentation board digitizer system, constructed and operative according to the teachings of the present invention;

5 FIG. 11 shows a second embodiment of the transmitting device;

FIGS. 12A and 12B show two different forms of the upper biasing element; and

FIG. 13 shows a second embodiment of the eraser.

### DESCRIPTION OF THE PREFERRED EMBODIMENTS

The present invention is of presentation board digitizer systems for use  
10 with presentation boards of all sizes which allow accurate reproduction of short pen strokes and which may be used with replaceable conventional pen elements.

The principles and operation of digitizer systems according to the present invention may be better understood with reference to the drawings and  
15 the accompanying description.

Referring now to the drawings, Figure 1 shows a presentation board digitizer system, generally designated **10**, constructed and operative according to the teachings of the present invention, showing a switch-over zone between regions with different groups of ultrasound receivers.

20 Generally speaking, system **10** features a presentation board **12**, which may be of any conventional type, provided with a plurality of ultrasound receiver assemblies **14**, **16** and **18**. Ultrasound receiver assemblies **14**, **16** and

18 are preferably mounted in a strip 20 adapted for convenient attachment to presentation boards of differing sizes and thicknesses. This attachment may be achieved through clamps or clips of any type. Strip 20 also features an infrared (IR) receiver 22. A cover (not shown) is preferably provided for shielding  
5 ultrasound receiver assemblies 14, 16 and 18 and IR receiver 22 from sound and radiation originating away from board 12. System 10 operates with a movable element having both ultrasound and infrared transmitters, an example of which will be described in detail below. The present position of the movable element is derived from the time-of-flight (TOF) of ultrasound signals from the  
10 movable element to the receiver assemblies by triangulation. The IR signal provides synchronization information, as well as carrying additional information such as, for example, the color of a pen being used.

In principle, two ultrasound receivers are sufficient to uniquely determine the position of a movable element in contact with board 12.  
15 However, in order to provide reliable ultrasound reception over the entire area of a large board, system 10 employs more than one set of receivers. Thus, in the system as illustrated, a first set of receivers is defined as the pair of ultrasound receiver assemblies 14 and 16, and a second set of receivers is defined as the pair of ultrasound receiver assemblies 16 and 18. Clearly, the first set of  
20 ultrasound receivers so defined is well positioned for receiving an ultrasound signal from the transmitter when the movable element is in a first region denoted A, and the second set of ultrasound receivers is well positioned for receiving the signal when the movable element is in a second region denoted C.

Thus, optimal precision and reliability is achieved by deriving the position of the movable element from the outputs of ultrasound receiver assemblies **14** and **16** when the movable element is in region A, and from the outputs of ultrasound receiver assemblies **16** and **18** when the movable element is in region C.

In order to avoid possible discontinuities in the tracking of the position of the movable element as it traverses board **12**, preferred embodiments of the present invention provide a switch-over zone, denoted B, between regions A and C. Within switch-over zone B, the current position of the movable element is derived based on a weighted function of the positions calculated from the outputs of the first and second sets of receivers. Preferably, the weighted function varies smoothly with position across switch-over zone B such that it approaches the value calculated from the first set of receivers when the movable element borders first region A and approaches the value calculated from the second set of receivers when the movable element borders the second region.

Figure 2 shows a typical variation of the weighting function with distance across board **12**. Here, plot **24** corresponds to the weighting factor applied to the first group of ultrasound receivers, and plot **26** corresponds to the weighting factor applied to the second group of ultrasound receivers. In this example, the variation within switch-over zone B is shown as linear. However, it should be appreciated that other more complex functions may be used as

desired. Within region A, plot 24 is preferably constant at 1 and plot 26 is zero, whereas within region B, these values are reversed.

It should be noted that calculation of the current position of the movable element according to the system described requires calculation of weighting factors which are themselves a function of position. This apparent circularity of calculation may be circumvented in a number of ways. Most simply, since the position is measured repeatedly at short intervals, it is reasonable to assume that the new current position is a relatively small distance from the previously measured position. It is therefore reasonable to employ the last measured position for calculating the weighting factors for the subsequent measurement. Alternatively, or for the purposes of making an initial measurement, an approximate measurement may be made with some arbitrary weighting factor such as, for example, 0.5 for each set.

Although the concept of the switch-over zone has been illustrated in a simple implementation with only two sets of receivers, the concept can clearly be extended to more complex arrangements of multiple sets of receivers, both colinearly and on opposite sides of a board. In the latter case, the weighting factor becomes a function of position in two dimensions, as will be clear to one ordinarily skilled in the art.

In addition to the switch-over zone algorithm, it is preferable that the ultrasound receivers are located sufficiently close to provide some degree of redundancy of measurement. This redundancy can then be employed (typically independent of the switch-over zone considerations) to provide a self test for

accuracy and to identify any erroneous measurements which may occur temporarily.

Specifically, if receivers **14**, **16** and **18** are collinear with equal spacing **A**, and the distance from each receiver as measured by TOF calculations is  $s_1$ ,  $s_2$  and  $s_3$ , respectively, simple trigonometry dictates that:

$$s_1^2 - 2s_2^2 + s_3^2 = 2A^2 \text{ (constant)}$$

By calculating this sum whenever three simultaneous TOF measurements are available, the system can continuously test that it is functioning within an acceptable margin of accuracy. In a case that a significant error is found, further statistically based self-analysis algorithms may be implemented to identify which receiver produced the erroneous reading and to temporarily exclude that receiver from position calculations.

Turning now to Figures 3 and 4, a preferred design of ultrasound receiver assembly, generally designated **30**, constructed and operative according to the teachings of the present invention, for use with presentation board digitizer systems will now be described. Assembly **30** may be used to advantage with a wide range of digitizer systems, including but not limited to system **10** described above.

Generally speaking, ultrasound receiver assembly **30** includes a first ultrasound receiver **32** located adjacent to the surface **34** of the presentation board, and a second ultrasound receiver **36** displaced from first ultrasound receiver **32** in a direction substantially perpendicular to surface **34**.

First and second ultrasound receivers **32** and **36** are connected so as to generate a total output signal corresponding to the instantaneous sum of the amplitudes of ultrasound signals which they receive. Typically, for simple transducers, this is achieved by connecting them in series such that their output  
5 voltages are additive.

Figure 4 shows a plot in polar coordinates of the variation of sensitivity of assembly **30** with angle of incidence in a plane perpendicular to the surface **34**. The phase differences between ultrasonic vibrations reaching the two receivers, when added, result in pronounced variation of the sensitivity of  
10 assembly **30** with angle of incidence, as shown. Specifically, the maximum sensitivity of assembly **30** occurs in a plane central to the main lobe of Figure 4 corresponding to a plane of symmetry between receivers **32** and **36**. Signals arriving at the two receivers which are incident from this plane necessarily have zero path and phase difference, thereby producing a maximum amplitude  
15 output signal. Reception from the  $n=1$  side lobes is preferably minimized by use of a cover element (not shown) which shields assembly **30** from sound incident at large angles from surface **34**.

By arranging assembly **30** as described, the plane of maximum sensitivity is oriented substantially parallel and adjacent to surface **34**. This is  
20 ideal for receiving signals incident from near the presentation board ( $S_2$ ). Conversely, assembly **30** exhibits greatly reduced sensitivity to signals ( $S_1$ ) incident from further away from the presentation board. These directional properties greatly help to isolate the ultrasound signals of importance to the

digitizer system, increasing the signal-to-noise ratio. This allows the use of lower transmitter intensities and/or larger boards, and solves problems caused by a wide range of common noise sources. It should be noted that the sensitivity profile of assembly 30 parallel to surface 34 remains substantially omnidirectional similar to the profile of an individual receiver.

Turning now to Figures 5-7, a preferred embodiment of a transmitter device, generally designated 40, constructed and operative according to the teachings of the present invention, for use with a drawing implement 42 in a digitizer system will be described. Transmitter device 40 may be used to advantage with a wide range of ultrasound based digitizer systems including, but not limited to, the presentation board digitizer systems described above.

Generally speaking, transmitter device 40 includes a housing 44 having a substantially cylindrical opening 46 which terminates at its lower end in an annular wedge surface 48 having a central bore 50. Drawing implement 42 is received within opening 46 with its operative tip 52 extending through bore 50.

Transmitter device 40 also includes a retainer 54 in the form of a cover attachable to the upper end of opening 46 to retain drawing implement 42 in position within housing 44. Retainer 54 features a spring element 56 for biasing drawing implement 42 towards annular wedge surface 48. An ultrasound transmitter 58 is mounted on the lower surface of housing 44 proximal to bore 50.

It is a particular feature of preferred embodiments of the transmitter device of the present invention that they can accommodate drawing implements

of a range of lengths and widths. To this end, spring element **56** adjusts to any variations in length, and biases drawing implement **42** towards the lower end of housing **44** to ensure a correct position for use. This biasing, in conjunction with the shape of annular wedge surface **48**, serves to center the front end of a drawing implement of any size or shape. In addition, spring element **56** is preferably provided with a shaped abutment surface **60** having features for centering the back end of a drawing implement. Typically, abutment surface **60** has an axial conical projection as shown for centering drawing implements by engaging a rear axial recess which is common to almost all presentation board pens. Alternatively, abutment surface **60** may be formed with a conical recess or other features for centering the back of a drawing implement.

It should be noted that the combination of annular wedge surface **48** and spring element **56** with abutment surface **60** serves to hold drawing implements of a range of lengths and widths in central alignment within cylindrical opening **46** without contacting the sides of housing **44**. This arrangement makes transmitter device **40** insensitive to variations in drawing implement width. The avoidance of frictional contact with the sides of housing **44** is also important for efficient operation of a contact-sensing microswitch, as will be described below.

It is a particular feature of certain preferred embodiments of the present invention that ultrasound transmitter **58** is formed as a substantially cylindrical piezoelectric transmitter element attached to the lower end of housing **44** around central bore **50**. This arrangement ensures that, when in use, the

cylindrical transmitter is coaxial with drawing implement **42**, circumscribing a part of drawing implement **42** proximal to operative tip **52**. As a result of the symmetry of this arrangement, TOF measurements of the position of drawing implement **42** are completely independent of axial rotation of transmitter device

5 **40**. Furthermore, the position of operative tip **52** can be determined very precisely by adding the radial dimension of transmitter cylinder **58** to the value calculated from the TOF.

Transmitter device **40** also typically features at least one element of an electromagnetic communications link, typically an IR transmitter **60**, and

10 preferably about four such transmitters spaced around the lower end of housing **44**. This ensures that at least one IR transmitter will be correctly oriented facing an IR receiver mounted on the presentation board at any time. It should be noted that a reversed arrangement in which an IR link is formed with a board-mounted transmitter and device **40** carries a receiver also falls within the scope

15 of the present invention. Furthermore, the IR link may be dispensed with entirely if three ultrasound receivers are used to calculate each position. However, the arrangement described is preferred for providing higher precision than a purely ultrasound-based system whilst avoiding the need for complex IR signal processing circuitry in the transmitter device. Additionally, the IR

20 transmitter allows transmission of extra information such as pen color and the like.

Ultrasound transmitter **58** and IR transmitters **60** are actuated under the control of electronic circuitry which is preferably battery powered. Both the

electronic circuitry and the battery are preferably located in a compartment 62 of housing 44.

Transmitter device 40 preferably also features a switch for detecting contact between operative tip 52 and the surface of a writing board. This switch is associated with the electronic circuitry and is employed to actuate ultrasound transmitter 58 and IR transmitters 60. Preferably, the switch is formed as a microswitch positioned to respond to changes in the force applied by drawing implement 42 against annular wedge surface 48. Figures 6A-6C show a preferred construction for such a microswitch, generally designated 64, constructed and operative according to the teachings of the present invention.

Microswitch 64 is formed from three functional layers. First, a base layer 66 provides the two terminals of the microswitch, a single peripheral contact 68 and a set of common contacts 70, spaced-apart around the center of base layer 66. On top of base layer 66 lies a layer of conductive resilient foam 72 having cut-out holes 74 opposite contacts 70. A third rigid conducting layer 76 lies above foam layer 72. Conducting layer 76 has small conductive downward projections 78 aligned with holes 74. An upper cover 80, integrally formed with annular wedge surface 48, attaches loosely to base layer 66 to unify the structure while allowing sufficient vertical motion for operation of the switch. Each layer has a central bore, together corresponding to bore 50 of Figure 5.

In a non-compressed state, conductive contact is made between peripheral contact 68 and foam layer 72 and between foam layer 72 and upper

conducting layer 76. However, the switch remains open since the thickness of foam layer 72 prevents contact between projections 78 and inner contacts 70. When pressure is applied to compress microswitch 64, foam layer 72 becomes compressed until projections 78 come into contact with inner contacts 70, thereby closing the switch. In principle, release of the pressure allows the foam layer to return to its initial state, thereby breaking the circuit. However, in practice, the relaxation response time of the foam material is typically quite slow. For this reason, a spring 82 is mounted between base layer 66 and upper conductive layer 76 such that, when the pressure is released, upper conductive layer 76 is lifted immediately so as to break the circuit.

It will be clear that, when drawing implement 42 is not in use, spring element 56 urges drawing implement 42 downwards against annular wedge surface 48 so as to close microswitch 64. When drawing implement 42 is used to draw on a presentation board, a force is exerted on operative tip 52 of drawing implement 42 towards housing 44, causing drawing implement 44 to recoil slightly against spring element 56. This reduces the pressure exerted on annular wedge surface 48 the circuit of microswitch 64 opens. The electronic circuitry of transmitter device 40 is responsive at least to opening of microswitch 64 to affect a signal transmitted by transmitter device 40.

Figure 6B shows microswitch 64 assembled, together with ultrasound transmitter 58 and IR transmitters 60. Figure 6C shows a pair of spring elements 84 which are mounted within annular wedge surface 48 so as to grip the end of a drawing implement inserted through central bore 50. This ensures

that the upper layer of microswitch **64** is sensitive to movements of drawing element **42**.

It should be noted that the structure described here for microswitch **64** is by way of example only. Alternative structures may be used such as, for example, a switch based on a piezoelectric pressure sensor or the like.

Finally with regard to microswitch **64**, it should be noted that correct operation of the switch depends on a degree of freedom of axial motion of drawing implement **42** against spring element **56**. For this reason, it is important that spring element **56** is not fully compressed when retainer **54** is attached. Figure 7 shows an example of a preferred structure for attachment of retainer **54** to housing **44**, in which lateral projections **86** engage channels **88** which are shaped to provide a margin of release **90** when fully engaged. Margin of release **90** is designed to be at least sufficient to allow an operative range of motion of microswitch **64**.

A second preferred embodiment of transmitter device **40** is shown in Figure 11. Similarly to the preferred embodiment shown in Figure 5, device **40** is intended for use with drawing implement **42**. Transmitter device **40** also features housing **44** with cylindrical opening **46**. However, cylindrical opening **46** now terminates at its lower end with a gasket **134**. Gasket **134** features a central bore **136**, through which operative tip **52** of drawing implement **42** extends.

In place of retainer **54**, transmitter device **40** features a different type of retainer, which is a holder **138**. Holder **138** is hingedly attached to the upper

end of housing **44** with a hinge **137**, and acts to hold drawing implement **42** substantially centered within opening **46**. Holder **138** locks onto housing **44** by a locking pin **139**. Holder **138** features a spring element **140** for biasing drawing implement **42** towards gasket **134**. A second spring element **142**,  
5 located near gasket **134**, preferably helps further bias and center drawing implement **42** within opening **46**. Preferably, spring element **140** is stronger than second spring element **142**. A cover **143** is also provided for drawing implement **42**.

In order to retain drawing implement **42** in the centered position, holder  
10 **138** preferably has an upper biasing element **144**. Upper biasing element **144** can be in one of two shapes, as shown in Figures 12A and 12B. Figure 12A shows upper biasing element **144** with an axial conical projection **146** for centering drawing implement **42** by engaging a rear axial recess **148** which is common to most presentation board pens. However, this embodiment is  
15 potentially restricted to use only with presentation board pens having axial recess **148** with a particular diameter, as axial recess **148** is not of uniform diameter between pens. Alternatively and preferably, upper biasing element **144** features a recess **150** into which the upper end of drawing implement **42** is inserted, as shown in Figure 12B. This second embodiment has the advantage  
20 of being usable with most presentation board pens, since the external diameter of these pens is generally uniform.

The combination of upper biasing element **144**, gasket **134** and spring elements **140** and **142** has the advantage of holding drawing implements of a

variety of lengths and external diameters in central alignment within cylindrical opening 46 substantially without contacting the sides of housing 44. As described above for Figure 5, the avoidance of frictional contact with the sides of housing 44 is also important for efficient operation of a contact-sensing microswitch 152.

Holder 138 also has a pressure-sensitive element 152, which has two parts, a pin 154 and a printed circuit board 156. Pin 154 contacts upper biasing element 144, sensing when contact is made between drawing implement 42 and the presentation board. In combination, these two parts allow transmitting device 40 to sense when contact has been made with the presentation board.

Transmitting device 40 also features ultrasound transmitter 58 and IR transmitter 60, similar to the embodiment shown in Figure 5. Ultrasound transmitter 58 and IR transmitters 60 are actuated under the control of electronic circuitry 158 which is preferably battery powered by a battery 160. Both electronic circuitry 158 and battery 160 are preferably located in holder 138 of housing 44.

Turning to Figures 8A-8C, a preferred transmission profile of transmitter device 40 will now be described. Figure 8A represents a contact profile of drawing element 42 as measured by microswitch 64 as a function of time. During a first period 100, drawing implement 42 is kept in contact with the presentation board for an extended period to draw a continuous shape. Then, during a second period 102, drawing implement 42 is used in a series of short, separate strokes to form a dashed line.

As mentioned above, the prior art digitizer systems suffer from a significant delay in picking-up the beginning of each pen stroke. This is because the transmitters are actuated each time pen contact is made and interrupted each time pen contact ceases. As a result, each pen stroke starts with a dead time during which the receiver system synchronizes and locks on to the transmitted signals. The results of this system are shown in Figure 8B. During period 100 the effects are not very serious. There is a small signal loss at the beginning of the period, but the great majority of the stroke is recorded well. During period 102, however, the system response time is comparable to the length of the pen strokes. As a result, the dashed line is almost completely lost.

To solve this problem, the present invention is preferably designed to maintain synchronization between transmitter device 40 and the receiver system for a given period after the end of each pen stroke. Typically, this is achieved by the electronic circuitry continuing to operate IR transmitters 60 for the given time interval after microswitch 64 ceases to indicate a force exerted on the outer housing towards the operative tip of the drawing implement. False drawing signals can be avoided either by the electronic circuitry disabling ultrasound transmitter 58 during the delay period, or by changing the content of the IR signal to indicate a non-contact pen state. The delay period is typically at least about half a second, and preferably between about 1 and about 2 seconds.

Figure 8C illustrates the response profile of transmitter device 40 as described. During an initial period of a single pen stroke, its response is not dissimilar from that of the prior art. However, when short repeated strokes are

encountered, transmitter device **40** maintains synchronization between successive strokes, thereby providing an accurate response immediately on switching of microswitch **64**.

Turning now to Figure 9, an eraser, generally designated **104**,  
5 constructed and operative according to the teachings of the present invention, for use with a presentation board digitizer system will be described. A major problem with eraser elements for use with digitizer systems is the common practice of employing only a part of the eraser surface. Since the digitizer is typically unable to distinguish between flat contact and edge contact of the  
10 eraser, the digitized image frequently shows a much greater erased area than has actually been cleared from the presentation board itself. To solve this problem, eraser **104** is constructed such that its eraser surface is self-orienting to lie parallel to the presentation board surface. This ensures that the contact area of the eraser element is always precisely defined.

15 Thus, eraser **104** has a handle **106** and an eraser element **108** which has a substantially flat, eraser surface **110**. Handle **106** and eraser element **108** are connected by a pivot joint **112**, typically in the form of a ball-and-socket, which has two degrees of rotational freedom. The use of pivot joint **112** ensures that, in use, eraser element **108** assumes an orientation with eraser surface **110**  
20 parallel to the presentation board surface substantially independent of the orientation at which handle **106** is held.

Eraser **104** also features transmitter device features analogous to those of transmitter device **40** described above. These include a cylindrical ultrasound

transmitter element **114**, a number of IR transmitters **116** and an electronic circuitry/battery block **118**. Connection of handle **106** to pivot joint **112** is through a sprung pin assembly **120**. A pressure sensing microswitch **122** is mounted in the seat of pin assembly **120** for sensing contact pressure between  
5 handle **106** and eraser element **108**. Wiring from electronic circuitry **118** to transmitters **114** and **116** is preferably located axially within pin assembly **120** and passing through pivot joint **112**.

Eraser surface **110** is preferably circular, and cylindrical ultrasound transmitter element **114** is preferably arranged such that its axis is aligned with  
10 the center of eraser surface **110**. By addition of the radius of the cylinder to the TOF measurements, this arrangement allows precise identification of the center of the circle of erasure, and hence of the entire area covered by eraser surface **110**. Eraser **104** thus provides a much higher degree of precision and determination of the erased area than can be achieved by prior art devices.

15 A second embodiment of an eraser **162** is shown in Figure 13. Eraser **162** is designed for erasing a small area, particularly an area of narrow width, and can thus be described as a “narrow-band eraser”. Similarly to eraser **104**, eraser **162** has a handle **164** and an eraser element **166** which has a substantially flat eraser surface **168**. However, handle **164** is connected to eraser element  
20 **166** by a pressure-sensitive element **170**. Pressure-sensitive element **170** includes a spring **172**, such that when at least a portion of eraser surface **168** contacts the presentation board, a signal is transmitted to a touch switch **174**. Touch switch **174** preferably includes a printed circuit board **176** and electrical

circuitry **178**, which enable touch switch **174** to identify when eraser surface **168** is contacting the presentation board. This is similar to pressure sensing microswitch **122** of eraser **104**.

A second method of identification of touching of the presentation board  
5 uses the following features of eraser **162**. Eraser surface **168** has two contact microswitches **180**, preferably located substantially at each end of eraser surface **168**, which are substantially similar in function to contact microswitch **64** of Figure 6. If only one contact microswitch **180** senses contact with the presentation board, only a small area will be erased, such as a letter, for  
10 example. If, however, both contact microswitches **180** sense contact with the presentation board, a zone with the length and width of eraser surface **168** will be erased.

Similarly to eraser **104**, eraser **162** also has transmitter device features. Specifically, eraser **162** has at least one, and preferably two, cylindrical  
15 ultrasound transmitters **182**, located in handle **164**, preferably substantially at each end of handle **164**. Since each ultrasound transmitter **182** is located in handle **164**, eraser **162** also features an ultrasound conductor tube **184** for each ultrasound transmitter **182**. Each ultrasound conductor tube **184** goes from handle **164** to eraser element **166**, such that the ultrasound signal from each  
20 ultrasound transmitter **182** is transmitted downward. Eraser **162** also has a reflector cone **186** for each ultrasound transmitter **182**. Reflector cone **186** is preferably located in eraser element **166**, reflecting the ultrasound waves in all directions.

Eraser **162** also has two infrared transmitters **188**, preferably located substantially at each end of handle **164**. Each infrared transmitter **188** has an infrared reflector **190**, also located in handle **164**, which serves a similar function as reflector cone **186**.

5           Although one particular embodiment of these transmitter device features has been described, it will be appreciated that a number of different embodiments are possible, substantially as described above for the transmitter device.

Turning now to Figure 10, this shows the principle of operation of a  
10 further embodiment of a transmitter device, constructed and operative according to the teachings of the present invention, for use with a presentation board digitizer system. This device is generally similar to transmitter device **40** described above except that it dispenses with microswitch **64**, instead identifying pen-board contact by transmission of vibrations through the board.

15           As mentioned earlier, digitizer systems employing through-the-board transmission suffer from poor accuracy and dependency on specific board design. However, they have a major advantage of inherent pen-board contact identification. The device of the present invention combines this feature with all the advantages of precision and independence from board design provided by  
20 air-borne ultrasound systems, using the through-the-board detection solely for contact detection.

Thus, this embodiment may be used with a presentation board system essentially similar to that of Figure 1, with the addition of a transducer

associated with the board (not shown) for detecting vibrations from the transmitter conducted through the board. The processor of the receiver system is then responsive to outputs from the air-borne ultrasound receivers to calculate a current position of the transmitter, and to the output from the board  
5 mounted transducer to identify contact between the drawing implement and the board, thereby identifying operative strokes of the drawing implement.

The principle of this system is shown clearly in Figure 10 in which plot  
130 represents the signal from one of the ultrasound receiver assemblies and plot 132 represents the signal from the board-mounted transducer. Plot 130  
10 shows a continuous sequence of pulses since the transmitters operate continuously as long as the pen is in use, according to this embodiment. Plot 132, on the other hand, only registers corresponding pulses during a period that the pen is in contact with the board. Although the signal quality of plot 132 is typically inferior, it is more than sufficient for identification of contact or non-  
15 contact conditions.

It will be appreciated that the above descriptions are intended only to serve as examples, and that many other embodiments are possible within the spirit and the scope of the present invention.

WHAT IS CLAIMED IS:

1. An ultrasound receiver assembly for use in a presentation board digitizer system, the receiver assembly comprising:

- (a) a first ultrasound receiver located adjacent to the surface of the presentation board; and
- (b) a second ultrasound receiver displaced from said first ultrasound receiver in a direction substantially perpendicular to the surface of the presentation board,

said first and second ultrasound receivers being connected so as to generate a total output signal corresponding to the instantaneous sum of the ultrasound signals received at each of said first and second ultrasound receivers such that the receiver assembly is most sensitive to ultrasound signals incident from a plane substantially adjacent to the presentation board.

2. The receiver assembly of claim 1, wherein said first and second receivers are connected in series.

3. In an ultrasound-based digitizing system for identifying the position of an ultrasound transmitter associated with an element movable relative to a surface, the system having at least three spaced apart ultrasound receivers associated with the surface, a method of analyzing outputs from the ultrasound receivers comprising the step of identifying as a current position a weighted centroid of at least a first calculated position derived from the outputs

of a first pair of the receivers and a second calculated position derived from the outputs of a second pair of the receivers, wherein the weighting varies as a continuous function of approximate position relative to the ultrasound receivers.

4. The method as in claim 3, wherein the ultrasound receivers are substantially collinear, and wherein the weighting varies linearly with distance in the direction of alignment of the ultrasound receivers over at least a given switch-over zone.

5. The method as in claim 3, wherein the weighted centroid approximates to said first calculated value when the movable element is within a first given region of the surface.

6. A presentation board digitizer system for digitizing operative strokes of a drawing implement carrying an ultrasound transmitter against the board, the system comprising:

- (a) at least two ultrasound receivers mounted relative to the board for receiving air-borne ultrasound signals;
- (b) a transducer associated with the board so as to detect vibrations from the transmitter conducted through the board; and
- (c) a processor responsive to outputs from said at least two ultrasound receivers to calculate a current position of the transmitter, said processor being additionally responsive to an

output from said transducer to identify contact between the drawing implement and the board, thereby identifying operative strokes of the drawing implement.

7. A transmitter device for use with a system for digitizing operative strokes of a hand-held drawing implement, the drawing implement having a body and an operative tip, the transmitter device comprising:

- (a) a housing having a substantially cylindrical opening terminating at a first end in a surface with a central bore, said housing receiving a portion of the body of the drawing implement with its operative tip extending from said central bore;
- (b) a retainer attachable to a second end of said opening to retain the drawing implement within said housing, said retainer having a spring element for biasing the drawing implement towards said surface; and
- (c) a transmitter mounted relative to said housing proximal to said central bore.

8. The transmitter device as in claim 7, wherein said housing further includes:

- (a) a microswitch actuated by changes in pressure exerted on said surface so as to be responsive to a force exerted on the operative tip of the drawing implement towards said housing; and

- (b) electronic circuitry responsive to said microswitch to affect operation of said transmitter at least when said microswitch indicates a force exerted on the operative tip of the drawing implement towards said housing.

9. The transmitter device as in claim 8, wherein said electronic circuitry operates said transmitter for a given time interval after said microswitch ceases to indicate a force exerted on said outer housing towards the operative tip of the drawing implement.

10. The transmitter device as in claim 9, wherein said given time interval is at least about half a second.

11. The transmitter device as in claim 8, wherein said transmitter transmits continuously, and wherein said electronic circuitry is responsive to said microswitch to change a signal transmitted by said transmitter while said microswitch indicates a force exerted on the operative tip of the drawing implement towards said housing.

12. The transmitter device as in claim 8, wherein said transmitter is an ultrasound transducer.

13. The transmitter device as in claim 12, further comprising elements of an electromagnetic communications link, said elements being associated with said electronic circuitry.

14. An ultrasound transmitter device for use with a system for digitizing the position of a hand-held drawing implement, the drawing implement having a central axis and an operative tip, the transmitter device comprising a substantially cylindrical piezoelectric transmitter element positioned coaxially with the drawing implement so as to circumscribe a part of the drawing implement proximal to the operative tip.

15. An eraser device for use with a presentation board digitizer system, the eraser device comprising:

- (a) a handle;
- (b) an eraser element having a substantially flat eraser surface; and
- (c) a pivot joint connecting between said handle and said eraser element, said pivot joint having two degrees of rotational freedom such that, in use, said eraser element assumes an orientation with said eraser surface parallel to the presentation board surface substantially independent of the orientation at which said handle is held.

16. A narrow-band eraser device for use with a presentation board digitizer system, the narrow-band eraser device comprising:

- (a) a handle;
- (b) an eraser element having a substantially flat eraser surface; and
- (c) a plurality of contact microswitches located on said eraser surface, such that when a portion of said eraser surface contacts the presentation board, at least one microswitch corresponding to said portion is activated and such that when substantially an entirety of said eraser surface contacts the presentation board, substantially all of said microswitches are activated.

17. The narrow-band eraser device of claim 16, further comprising a plurality of ultra-sound transmitters and a plurality of infra-red transmitters for identifying contact with the presentation board.

18. The narrow-band eraser device of claim 17, further comprising at least one reflector for each of said transmitters.

19. The narrow-band eraser device of claim 16, further comprising a pressure-sensitive element for identifying contact with the presentation board.

### ABSTRACT OF THE DISCLOSURE

A presentation board digitizer system for large boards preferably employs at least three spaced-apart ultrasound receivers assemblies. A current position of an ultrasound transmitter is assigned as a weighted centroid of time-of-flight position measurements based on at least two pairs of receiver assemblies. The weighting used varies as a function of the position of the transmitter across the board. A preferred structure of an ultrasound receiver assembly for use in the system employs a pair of ultrasound receivers arranged side-by-side in a line perpendicular to the surface of the presentation board. The receivers are connected so as to generate a total output signal corresponding to the instantaneous sum of the ultrasound signals received at each, such that the receiver assembly is most sensitive to ultrasound signals incident from a plane adjacent to the presentation board. Also described are a transmitter device for use with a conventional pen in which the ultrasound transmitter is a cylindrical element lying coaxial with the pen and adjacent to its tip, and a jointed eraser structure.

FIG. 1

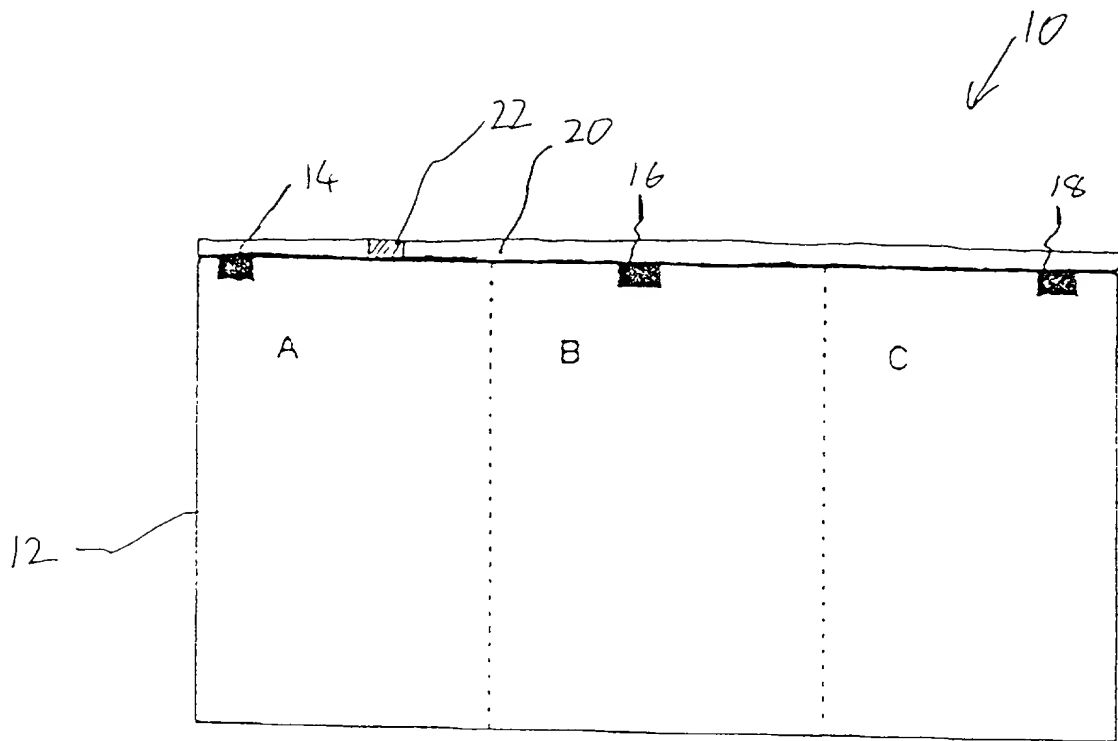


FIG. 2

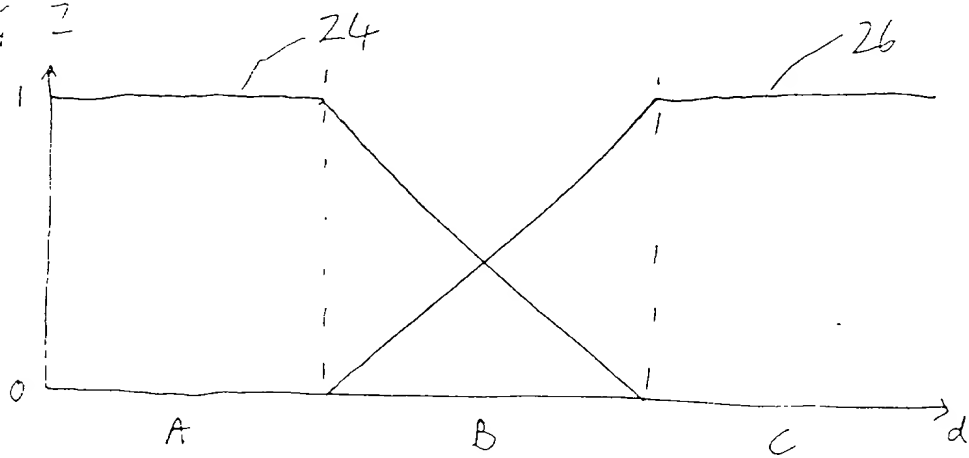


FIG. 3

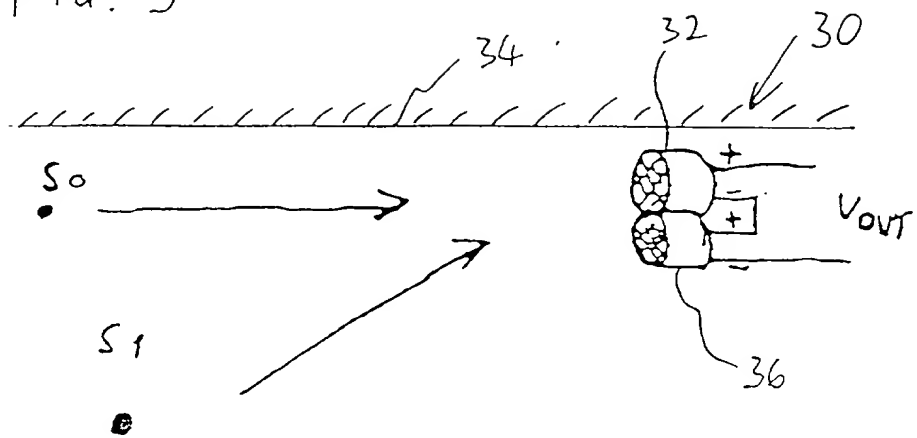


FIG. 4

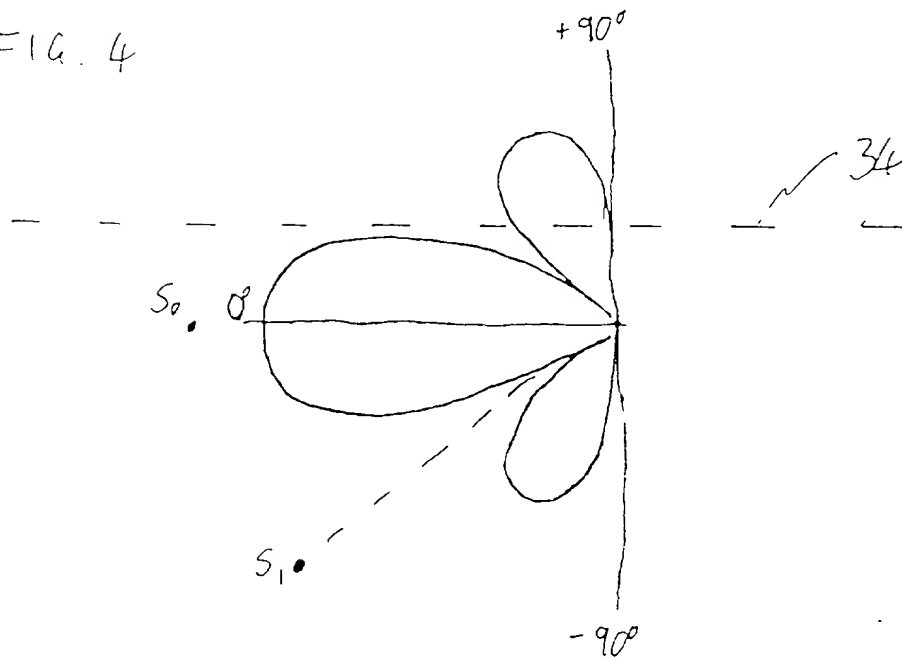


FIG. 5

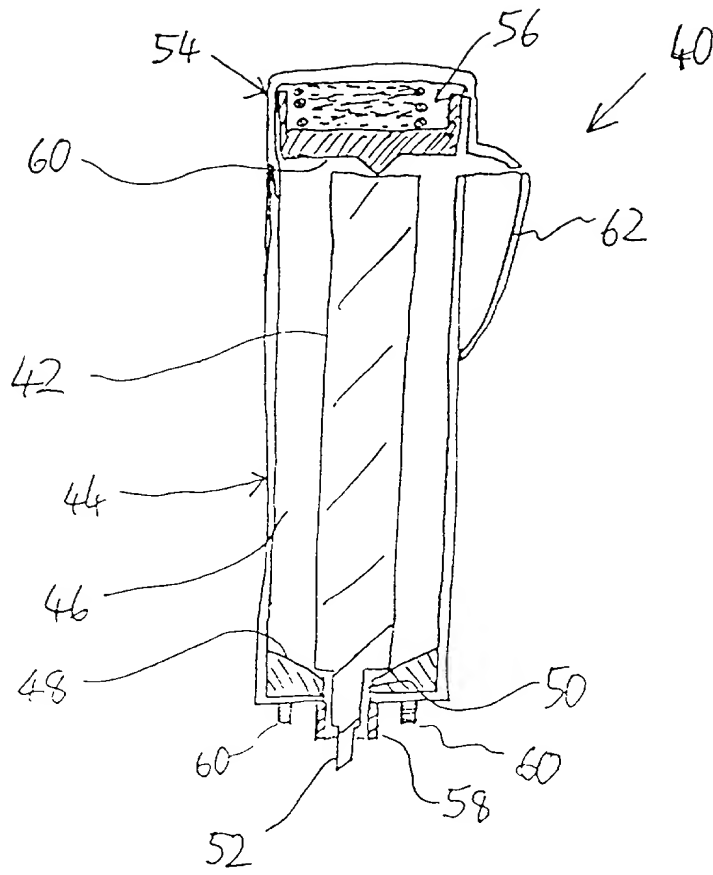


FIG 6A

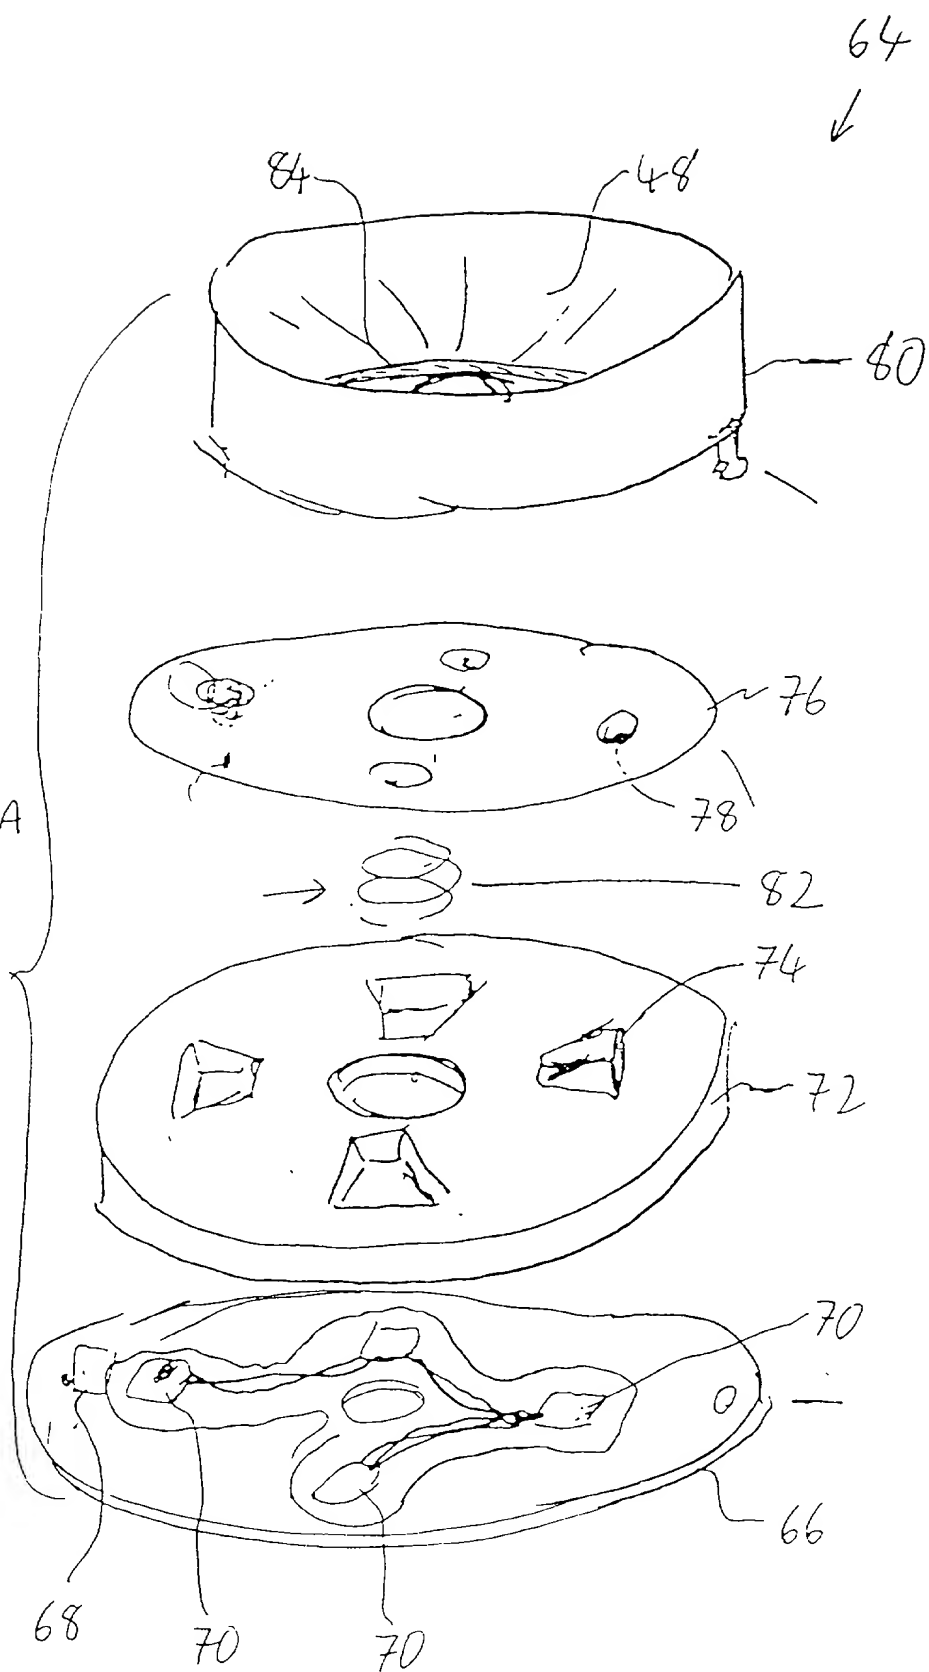


FIG. 6B

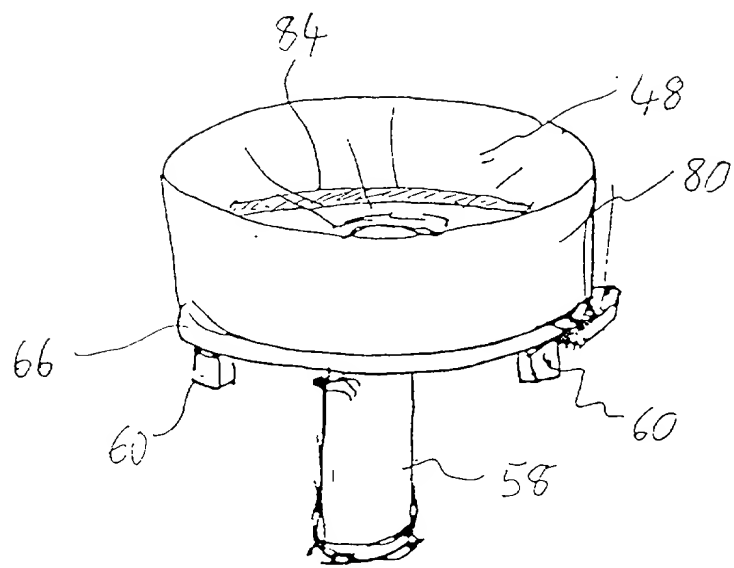


FIG. 6C

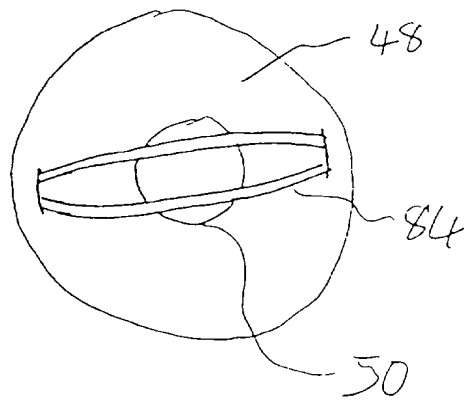
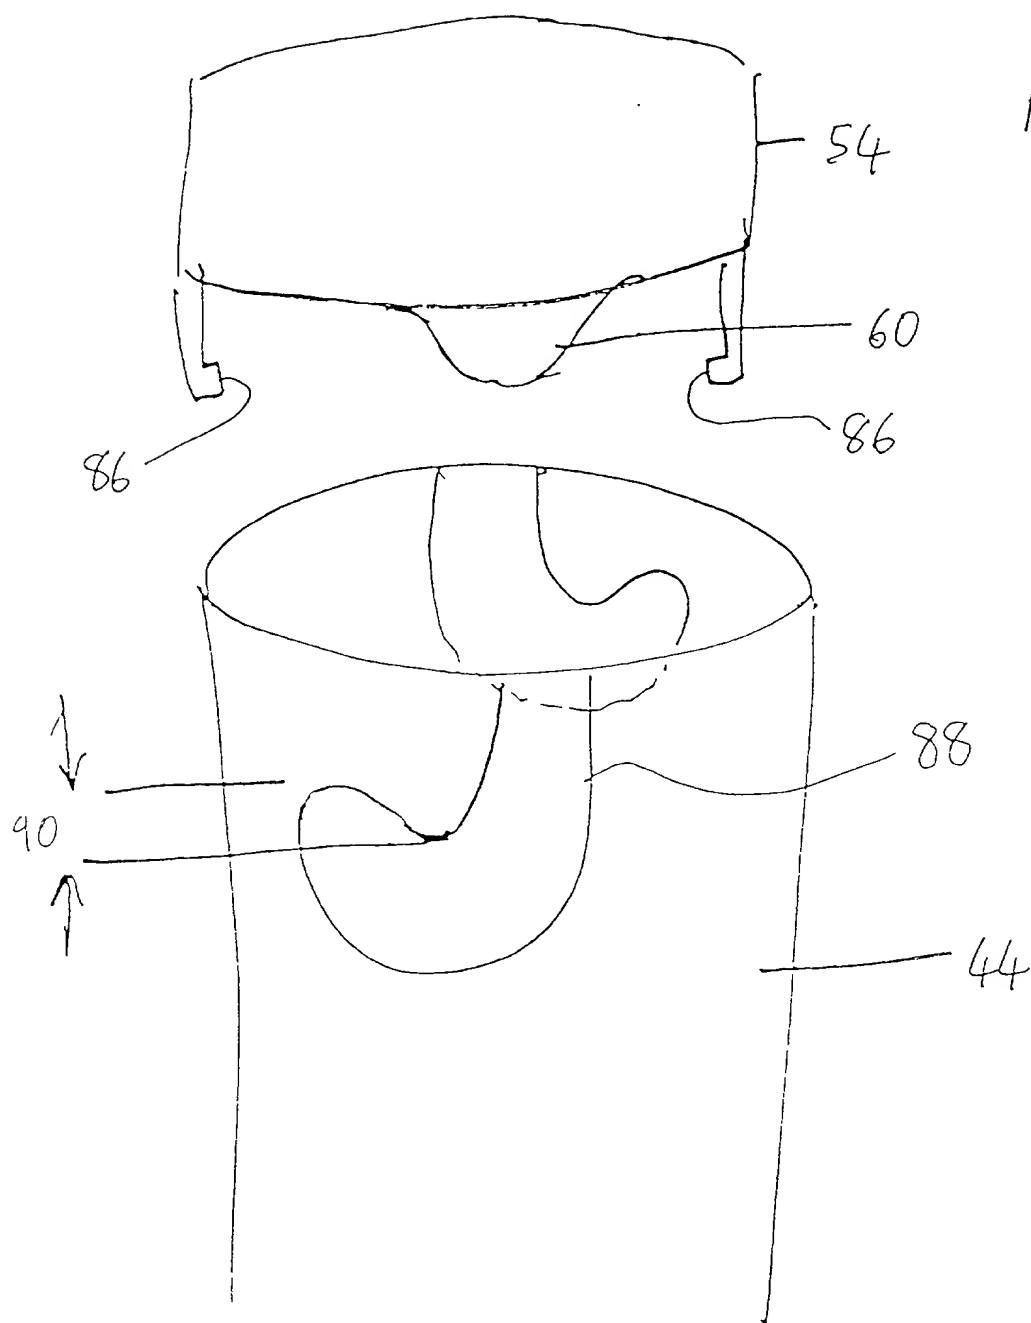


FIG. 7



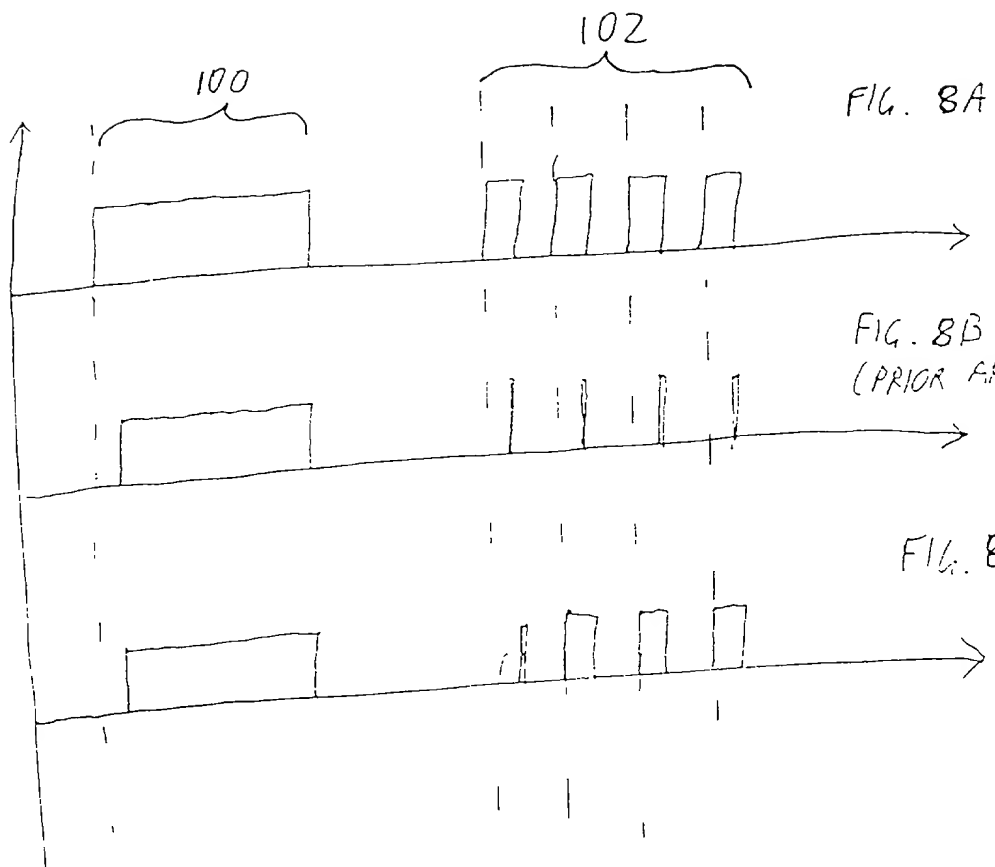


FIG. 9

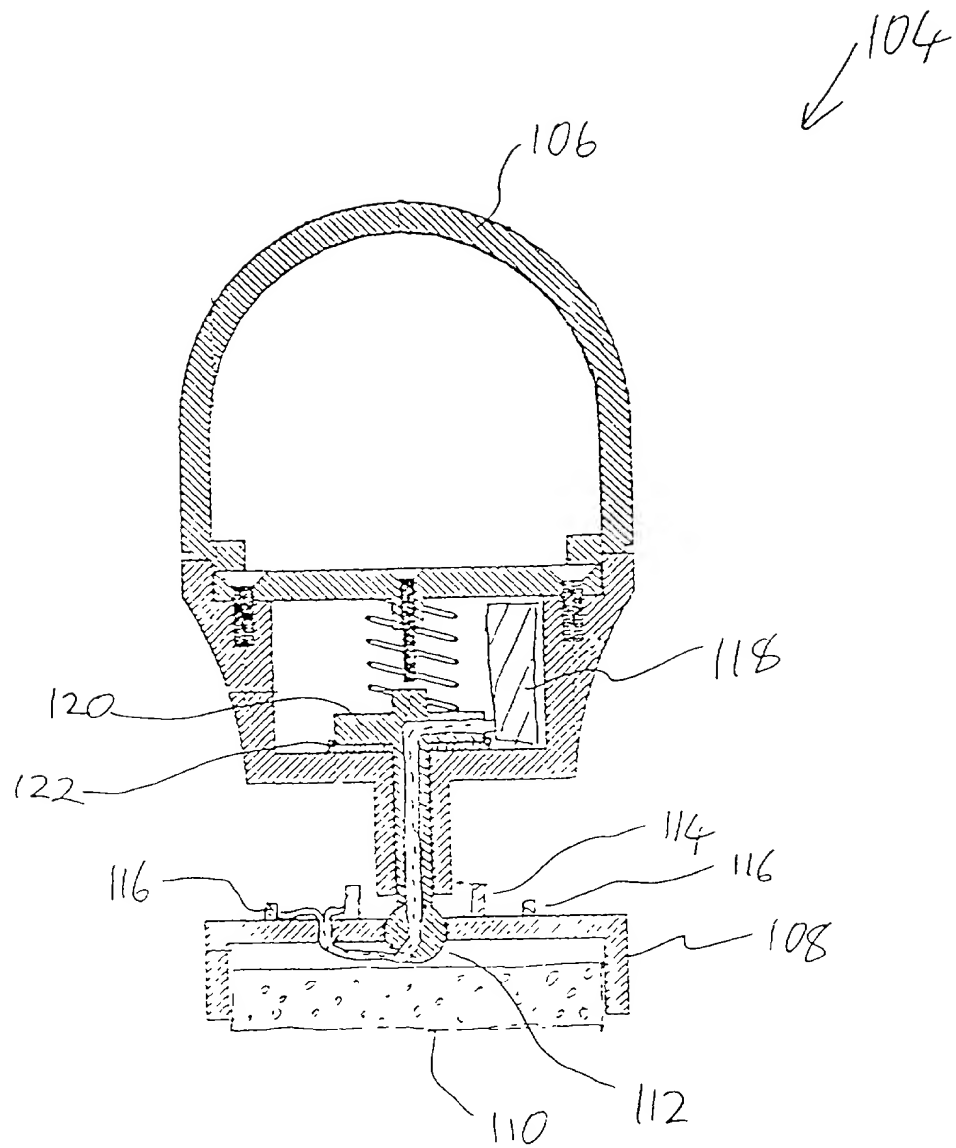
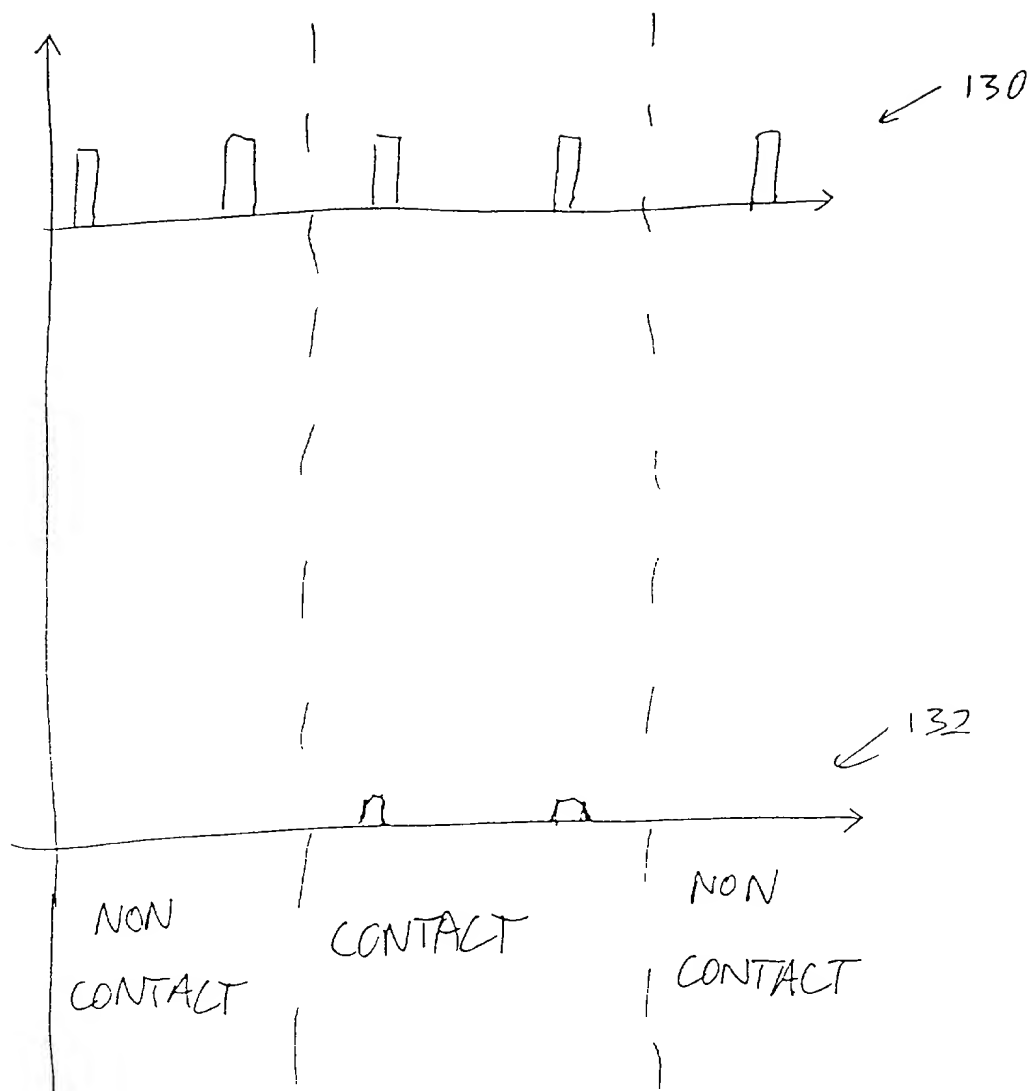


FIG. 10



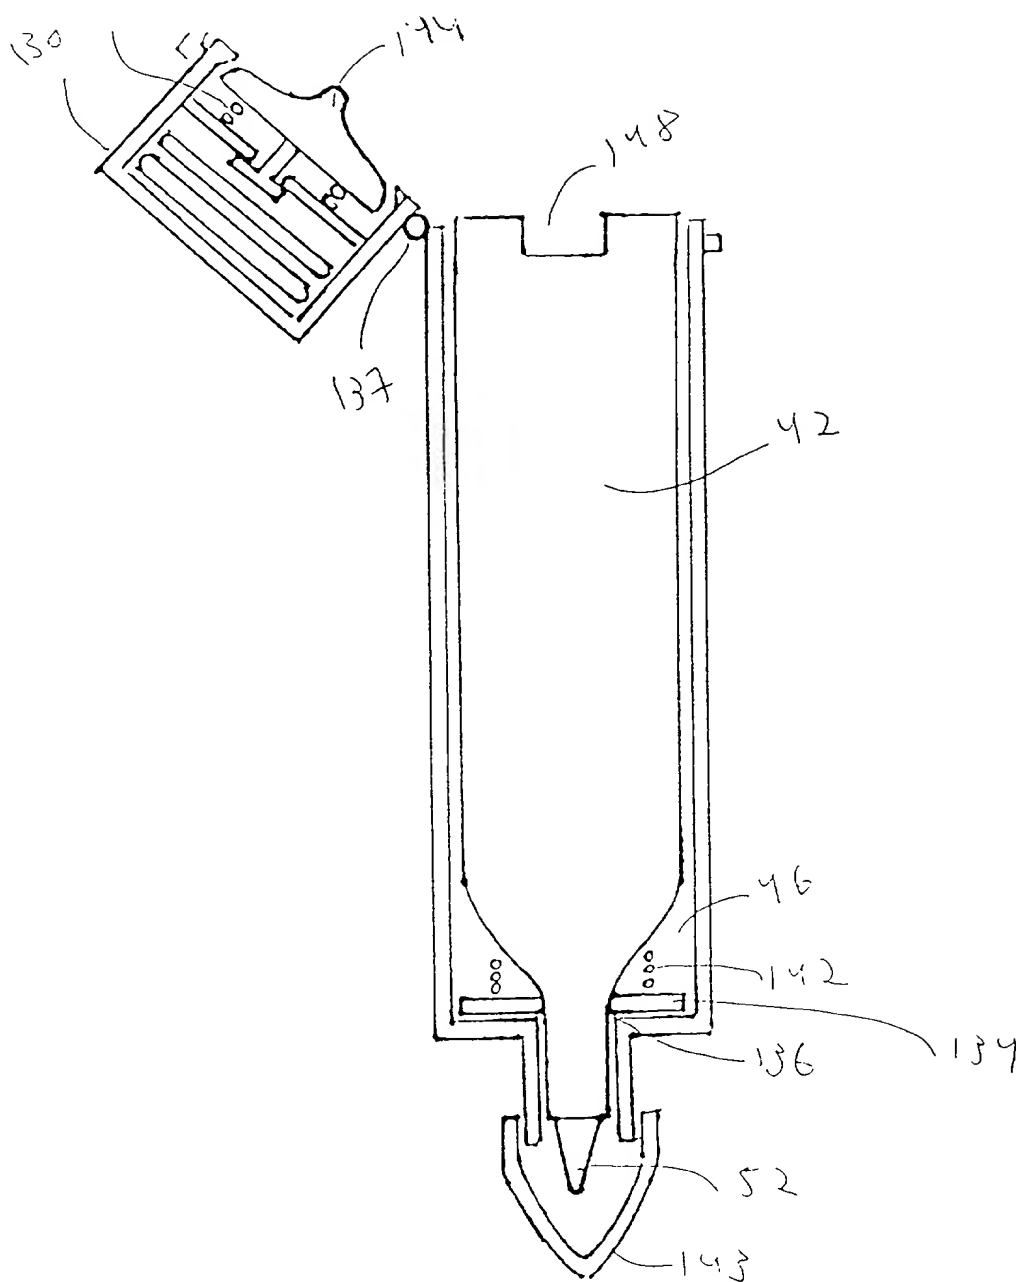


Figure 11

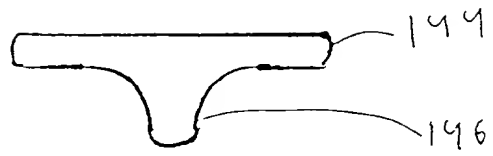


Figure 12A

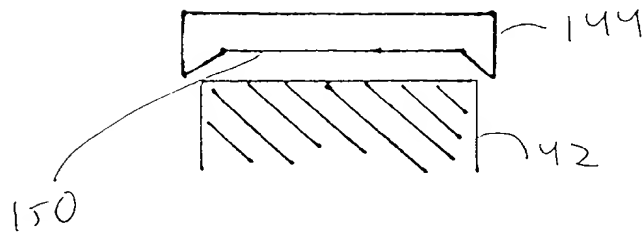


Figure 12B

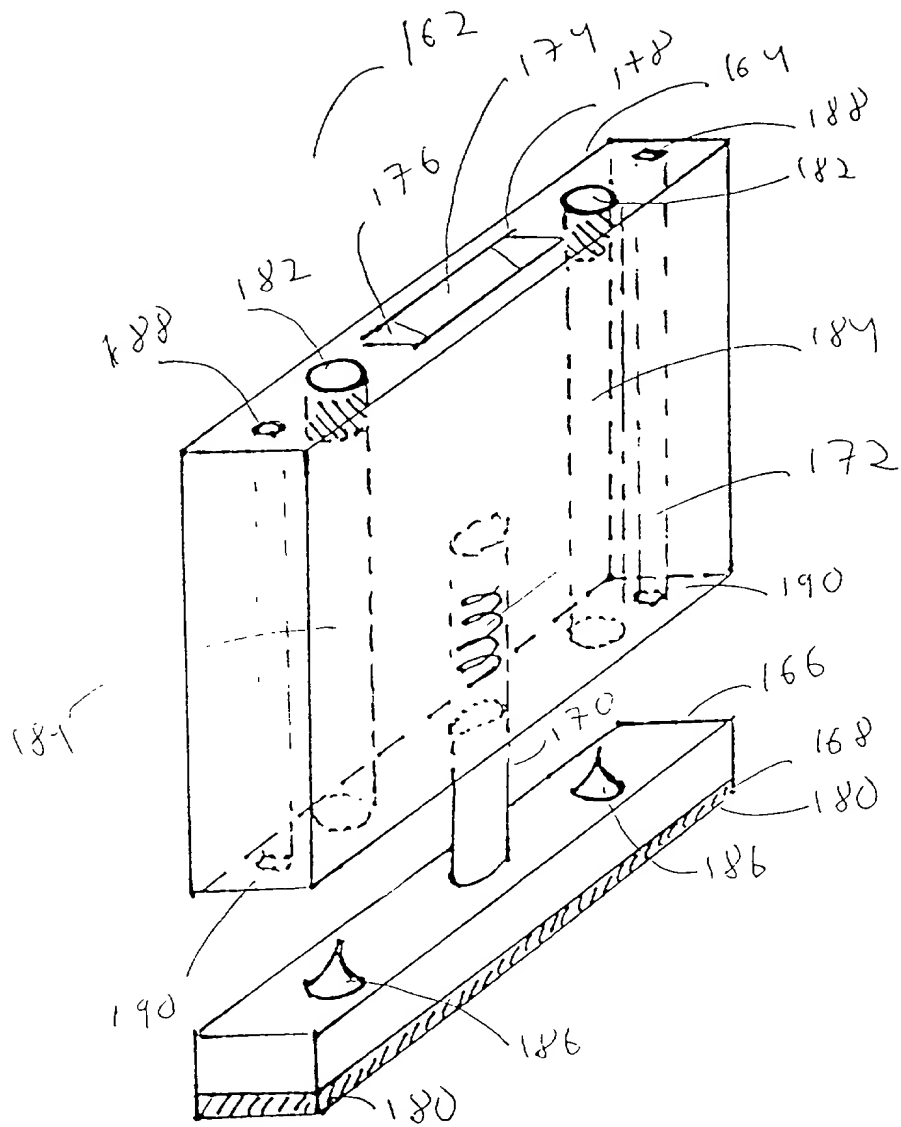


Figure 13

Attorney Docket: 172/19  
page 1 of 1

Combined Declaration For Patent Application and Power of Attorney

As a below named inventor, I hereby declare that:

My residence, post office address and citizenship are as stated below next to my name;

I believe I am the original, first and sole inventor (if only one name is listed below) or an original, first and joint inventor (if plural names are listed below) of the subject matter which is claimed and for which a patent is sought on the invention entitled PRESENTATION BOARD DIGITIZER SYSTEMS, the specification of which (check one) ☒ is attached hereto.

☐ was filed on \_\_\_\_\_ as Application Serial No. \_\_\_\_\_ and was amended on \_\_\_\_\_. I hereby state that I have reviewed and understand the contents of the above identified specification, including the claims, as amended by any amendment referred to above.

I acknowledge the duty to disclose information which is material to the patentability of this application in accordance with Title 37, Code of Federal Regulations, § 1.56(a).

I hereby claim foreign priority benefits under Title 35, United States Code, § 119 of any foreign application(s) for patent or inventor's certificate listed below and have also identified below any foreign application for patent or inventor's certificate having filing date before that of the application on which priority is claimed:

Prior Foreign Application(s)	Priority Claimed
<u>120417</u> (number)	<u>IL</u> (Country)
<u>10-Mar-97</u> (Day, Month, Year Filed)	<input checked="" type="checkbox"/> Yes <input type="checkbox"/> No
<u>          </u> (number)	<u>          </u> (Country)
<u>          </u> (Day, Month, Year Filed)	<input type="checkbox"/> Yes <input type="checkbox"/> No
<u>          </u> (number)	<u>          </u> (Country)
<u>          </u> (Day, Month, Year Filed)	<input type="checkbox"/> Yes <input type="checkbox"/> No

I hereby claim the benefit under Title 35, United States Code, § 120 of any United States Application(s) listed below and, insofar as the subject matter of each of the claims of this application is not disclosed in the prior United States application in the manner provided by the first paragraph of Title 35, United States Code, § 112, I acknowledge the duty to disclose material information as defined in Title 37, Code of Federal Regulations, § 1.56(a) which occurred between the filing date of the prior application and the national or PCT international filing date of this application:

<u>NONE</u> (Application Serial No.)	<u>          </u> (Filing Date)	<u>          </u> Status (patented, pending, abandoned)
<u>          </u> (Application Serial No.)	<u>          </u> (Filing Date)	<u>          </u> Status (patented, pending, abandoned)

I hereby appoint the following attorneys, with full power of substitution, association, and revocation, to prosecute this application and to transact all business in the Patent and Trademark Office connected therewith.

Mark M. Friedman Registration No. 33,883

Address all Correspondence to:

DR. MARK FRIEDMAN LTD.  
c/o ANTHONY CASTORINA  
2001 JEFFERSON DAVIS HIGHWAY  
SUITE 207  
ARLINGTON, VIRGINIA 22202

Direct all telephone calls & faxes to:  
ROBERT SHEINBEIN  
Phone (703) 415-1581  
Fax (703) 415-4864

I hereby further declare that all statements made herein of my own knowledge are true and that all statements made on information and belief are believed to be true; and further that these statements were made with the knowledge that willful false statements and the like so made are punishable by fine or imprisonment, or both, under Section 1001 of Title 18 of the United States Code and that such willful false statement may jeopardize the validity of the application of any patent issued thereon.

*FULL NAME OF SOLE OR FIRST INVENTOR GIDEON SHENHOLZ	INVENTOR'S SIGNATURE <i>[Signature]</i>	DATE 10 FEB 98
RESIDENCE 2 HAEKOSHI, 64073 TEL AVIV, ISRAEL	CITIZENSHIP ISRAELI	
POST OFFICE ADDRESS 2 HAEKOSHI, 64073 TEL AVIV, ISRAEL		
*FULL NAME OF SECOND INVENTOR YITZHAK ZLOTOR	INVENTOR'S SIGNATURE <i>[Signature]</i>	DATE 10 FEB 98
RESIDENCE 4 HAAVODA, 58504 HOLON, ISRAEL	CITIZENSHIP ISRAELI	
POST OFFICE ADDRESS 4 HAAVODA, 58504 HOLON, ISRAEL		
*FULL NAME OF THIRD INVENTOR	INVENTOR'S SIGNATURE	DATE
RESIDENCE	CITIZENSHIP ISRAELI	
POST OFFICE ADDRESS		